

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):


- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

Installation code
PC-587857-A

User Information

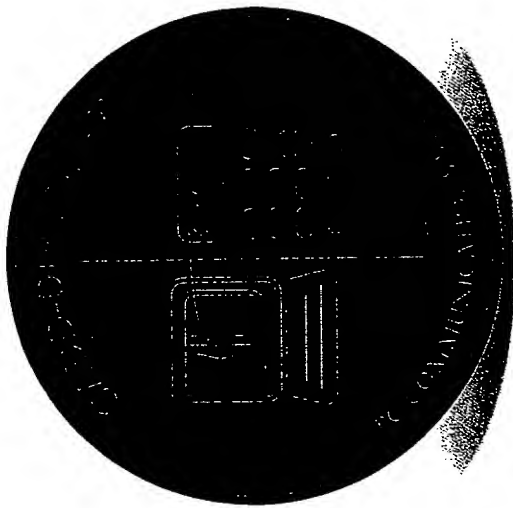

Deltec

SIMS Deltec, Inc., St. Paul, MN 55112 U.S.A.



Deltec®, CADD-Prizm®, and CADD® are registered trademarks of SIMS Deltec, Inc.
CADD-Diplomat™ and CADD-Ambassador™ are trademarks of SIMS Deltec, Inc.

© 1998 SIMS Deltec, Inc. All rights reserved. Printed in U.S.A.
SIMS Deltec, Inc., St. Paul, MN 55112 U.S.A.

3/98
40-3911-01A

CADD-DIPLOMAT™

PC COMMUNICATIONS SYSTEM

EXHIBIT

A

Labels

This guide pertains only to the CADD-Diplomat™ PC Communications System. For detailed instructions, specification, warnings, warranty, and additional information on operating the CADD-Prizm® pump, please refer to the Operator's Manual supplied with the pump.

Technical Assistance

If you have questions while installing the software, please contact Clinical Services at 800-426-2448 between the hours of 8:00 a.m. and 5:00 p.m. CST. If you have comments or questions concerning the operation of the modem or other computer components, please refer to the product literature provided with the modem or component for the appropriate Customer Service number.

Clinical Assistance

If you have comments or questions concerning the operation of the CADD-Diplomat PC Communications System, please call this number: 800-426-2448. Our staff is available to help clinicians twenty-four hours a day with the operation of the CADD-Diplomat Pump Communications System.

Table of Contents

Equipment and software requirements	1
Equipment the patient needs	2
Modem Information	2
Modem Types	2
Installing the modem	2
Installing the Software	3
CD-ROM	3
Floppy Disks	3
Using On-line Help	4
Connecting with a Modem	4
Direct Connect	6

Equipment and software requirements

- ◇ A 486 or faster PC compatible computer
(if using an internal modem, a 16 Bit ISA slot must be available)
- ◇ A modem, SVD recommended

NOTE: *The modem supplied by Deltac is highly recommended. Performance is best with an external modem and analog telephone. Results with other configurations may vary.*

- ◇ 8 MB RAM (minimum)
- ◇ 3.5" disk drive or CD-ROM drive
- ◇ Hard drive with at least 20 MB available
- ◇ Windows 95
- ◇ Mouse for electronic pointing or similar device
- ◇ Available RS232 serial port if external modem or direct connection desired
- ◇ A CADD-Diplomat™ PC Communications System (including software, AC adapter (for external modem), PC cable, and telephone line wire)
- ◇ An analog telephone with cord is recommended. Check with your institution to ensure an analog phone is available to use.
- ◇ A modular-type wall telephone jack with an analog phone line

CAUTION: *DO NOT connect the modem to a digital phone line. Before connecting the modem to a telephone line, ensure that it is analog. The higher voltages in a digital telephone system can damage the modem.*

Equipment the patient needs

- A CADD-Ambassador™ Pump Communications System (including SVD modem, AC adapter, interface cable, and telephone line wire)
- CADD-Prizm® pump, Model 6101 or Model 6100 installed with software version 0254-01E or newer

Once you have the software installed, you can refer to the on-line help to assist the patient in setting up the equipment. See "Preparing Patient for Communications" help topic.

Modem Information

Modem Types

Two types of modems are Simultaneous Voice/Data (SVD) and non-SVD. A SVD modem allows you to talk to the patient on the telephone during communications, because it can transfer data and voice at the same time. With a non-SVD modem you cannot talk to the patient, because it can only transfer data during communications. The CADD-Diplomat PC Communications System is designed to be used with a SVD modem, which is the type of modem that may be purchased from SIMS Deltec. Both of these modem types can be internal, inside the computer case, or external, outside of the computer case.

Installing the modem

If the modem is not already installed, install the modem according to the manufacturer's instructions.

After setting up the modem, test it to make sure it is working properly.

Installing the Software

CD-ROM

1. Insert the CD-ROM in the CD-ROM drive.
2. Click the Start button and select Run.
3. In the open box, type "e:\setup" (or replace "e" with the appropriate letter for the CD-ROM drive on your system).
4. Click OK.
5. Follow the instructions on the screen.

Floppy Disks

1. Insert the floppy disk labeled "Disk #1."
2. Click the Start button and select Run.
3. In the open box, type "a:\setup" and click OK.
4. Follow the instructions on the screen.

Specific instructions for how to use the CADD-Diplomat PC Communications System are included in the help screens provided with the software. Once the software is installed and the modem is functioning, you can use on-line help, or follow instructions provided with some functions on the screen.

Using On-line Help

CADD-Diplomat PC Communications has two kinds of help.

"How to . . ." topics, found under the help menu item on the main screen of the program, describe the basic features of CADD-Diplomat PC Communications. The green, underlined words or phrases within the help topics are hyperlink topics. When you click on a hyperlink topic, you jump to that topic in the help screens.

Balloon Help consists of small pieces of information enclosed in "bubbles" like those used for indicating the speech of comic strip characters. To see an explanation of an item on the computer screen, use the mouse to position the cursor over the item on the screen without clicking on it.


NOTE:

- ◊ Not everything on the screen will have balloon help available.
- ◊ The help screens cannot be accessed while connecting and disconnecting communications with the pump.

Connecting with a Modem

You may connect your PC to the pump remotely with a modem. Once a connection is established, the patient's screens appear on your PC so you can view, troubleshoot, or program the pump as through you are actually working with the patient's pump. A connection can be established regardless of whether the patient's pump is running, stopped, or sounding an alarm (except a pump error).

An example of equipment set up with an external modem is shown at right.

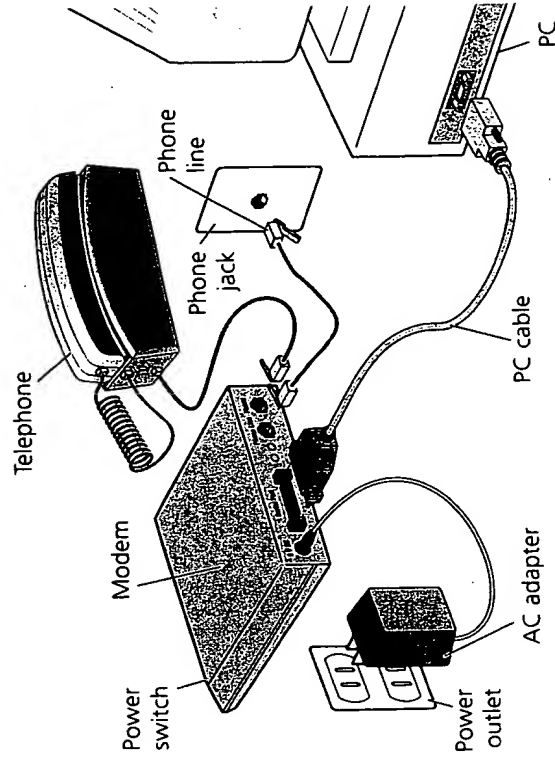

Direct Connect

If you want to run reports from a pump you have in your office, you can connect the pump to the PC directly using a Deltec Interface Cable and a NULL modem cable. The interface cable allows connection between the pump and NULL Modem cable. The NULL modem, which allows the pump and the computer to connect without a modem, makes the modem null, or unnecessary. It attaches to the PC.

1. Attach the NULL modem cable (the cable with 25 pin holes in one end and 9 pin holes in the other end) to the interface cable. The end with 25 pin holes fits with the end of the interface cable with 25 pins.
2. Connect the end of the NULL modem cable with 9 pin holes to the computer's serial port and tighten the screws. Consult your computer's manual if you are not sure which connector to use.

NOTE: Connecting directly to the serial port may not work in some situations or may require additional set up. Consult the product literature supplied with the computer for troubleshooting information. Some examples of problems follow:

- The port is used by the modem.
- The port is used by a mouse.
- The port is turned off.
- The port is configured for IR communications.

